

& obstructive sleep apnea

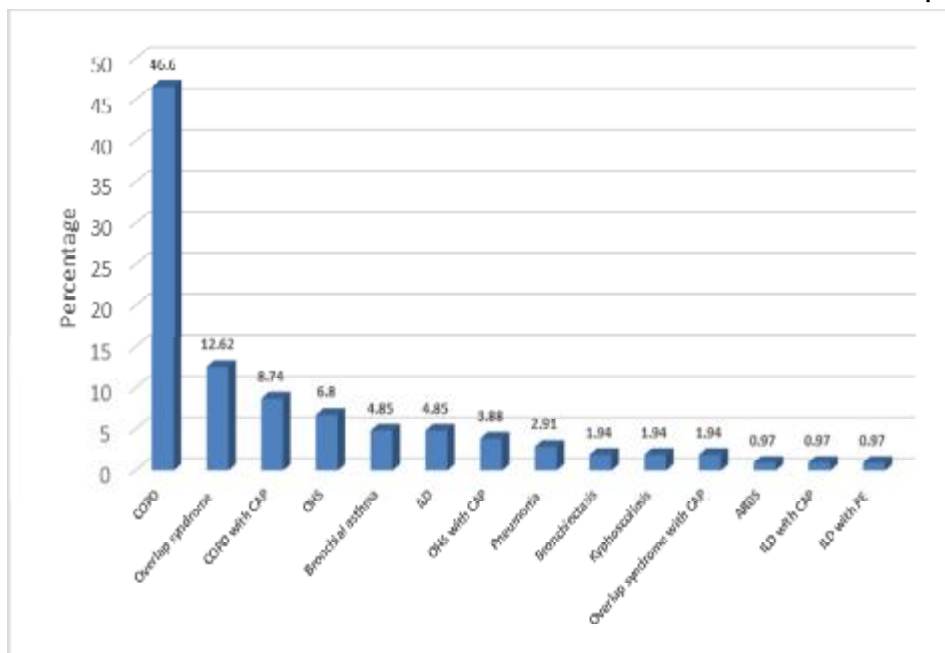


Fig.(1) : Diagnosis of studied population

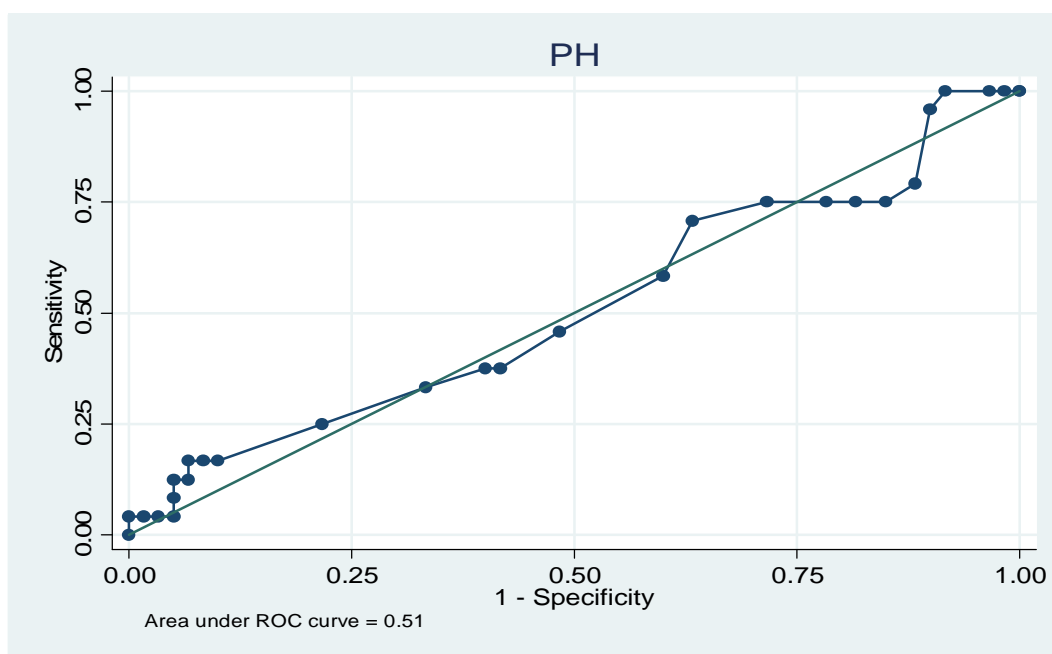


Fig (2): Area under receiving operating characteristic curve for PH to predict failure The optimum cut off level was ≤ 7.22 with 25.0% sensitivity and 85.0% specificity, with an AUC of 0.51 (CI [0.38-0.60]).